




Thermal Imaging Riflescope

# **THERMIION 2 LRF XQ50 PRO**

Reticle Catalogue





## Non-scalable reticles

The values of the non-scalable reticles are correct in the following cases:

- when the magnification of the scope is set to minimum
- when "picture in picture" is activated

+

**D50i**



**C50i**



**X54i**



**H50i**



**X50i**



**T54**



**M58i**



**X51Fi-300**



**M56Fi (Mil-Dot)**




**M57Fi (Mil-Dot)**

## Scalable reticles


Reticle parameters apply to all magnifications



# D50i

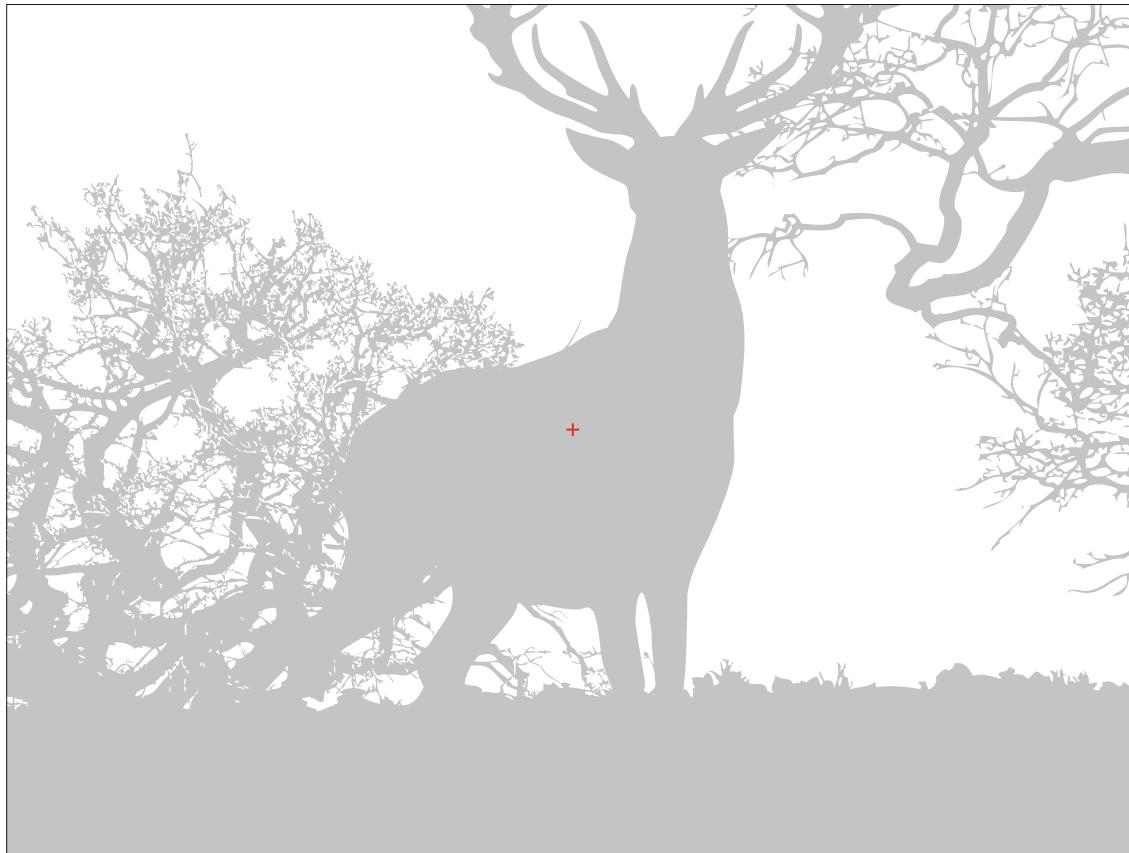

**Reticle parameters**  
(for minimum magnification)

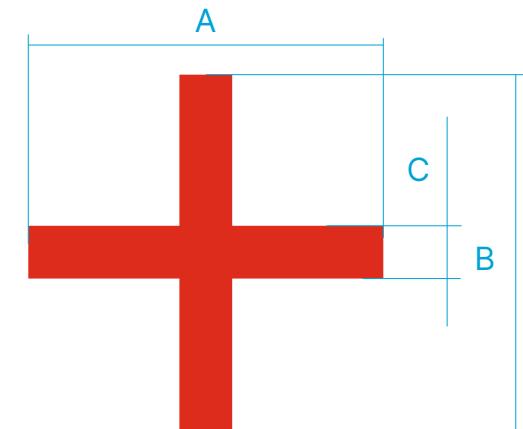

	MOA	cm @ 100 m
Section A	3.1	9
Section B	3.1	9
Section C	0.4	1.2


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


[TO CONTENT](#)



# C50i

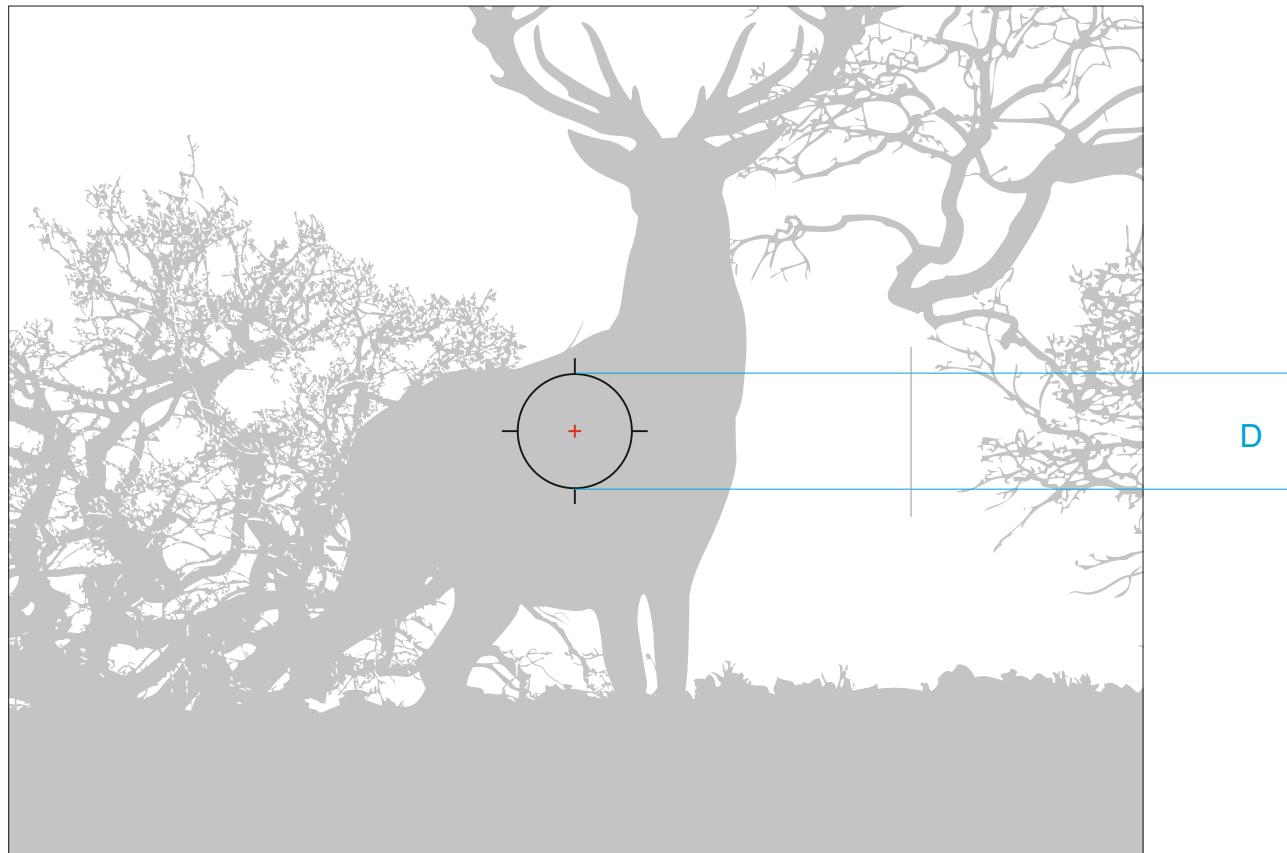

**Reticle parameters**  
(for minimum magnification)

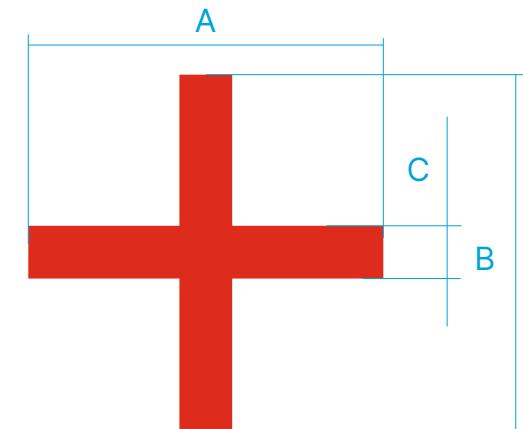

	MOA	cm @ 100 m
Section A	3.1	9
Section B	3.1	9
Section C	0.4	1.2
Section D	34.4	100


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


[TO CONTENT](#)



# X54i

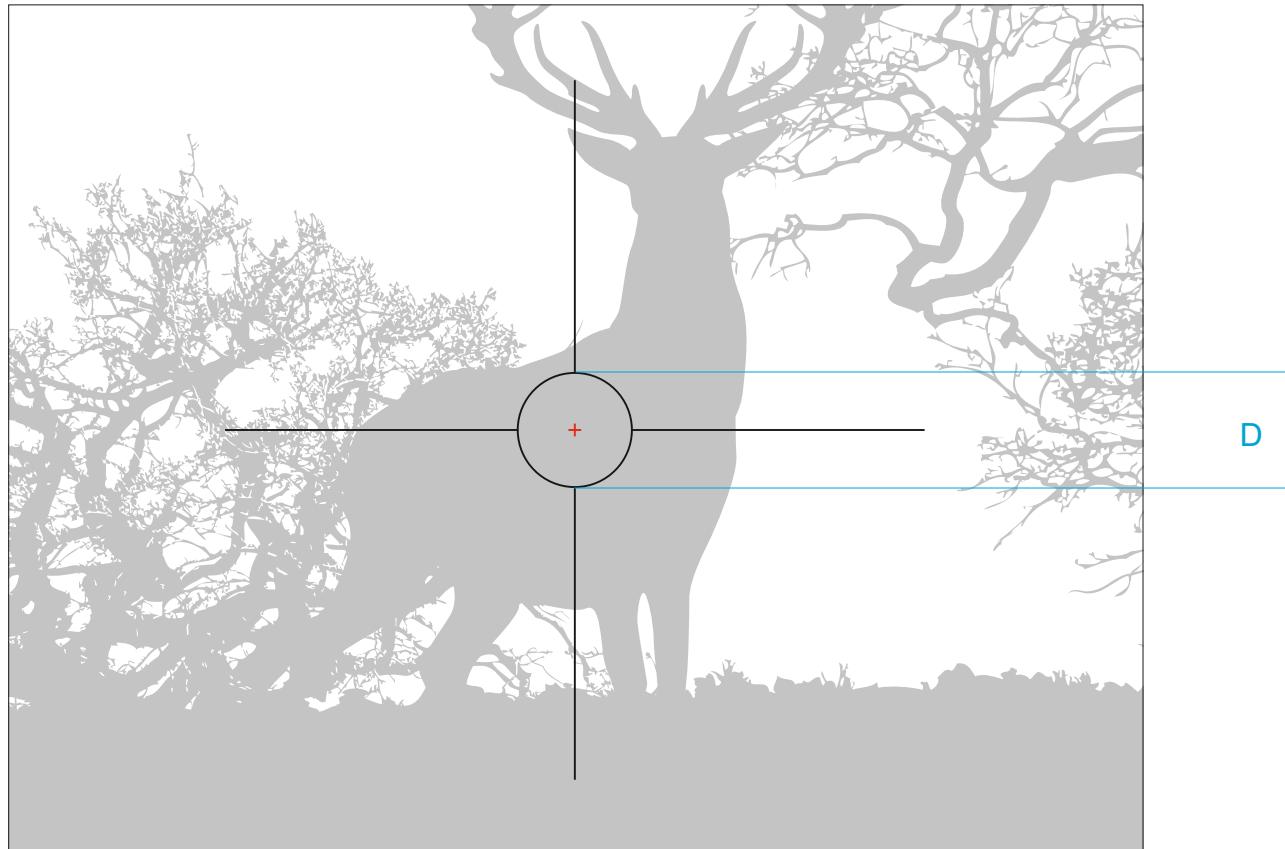

**Reticle parameters**  
(for minimum magnification)

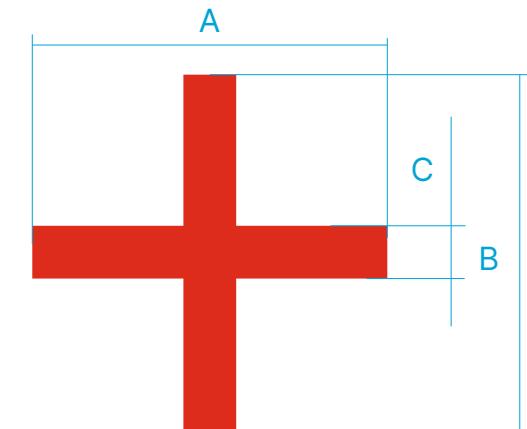

	MOA	cm @ 100 m
Section A	3.1	9
Section B	3.1	9
Section C	0.4	1.2
Section D	34.4	100


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


[TO CONTENT](#)



# H50i

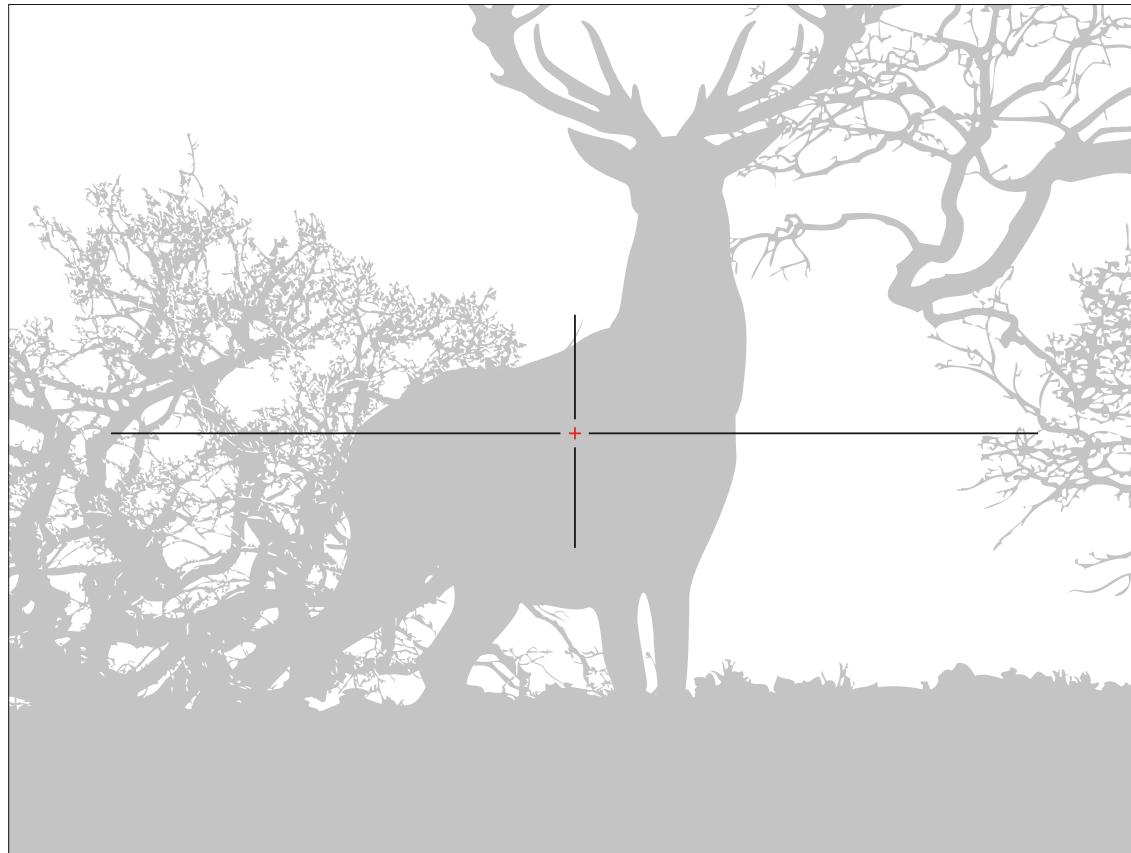

**Reticle parameters**  
(for minimum magnification)

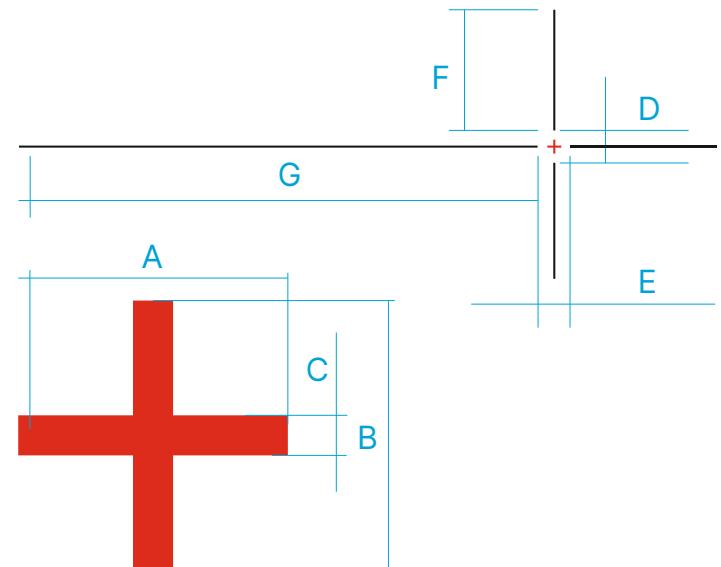

	MOA	cm @ 100 m
Section A	3.1	9
Section B	3.1	9
Section C	0.4	1.2
Section D	20	58
Section E	20	58
Section F	34	99
Section G	128	372


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


[TO CONTENT](#)



# X50i

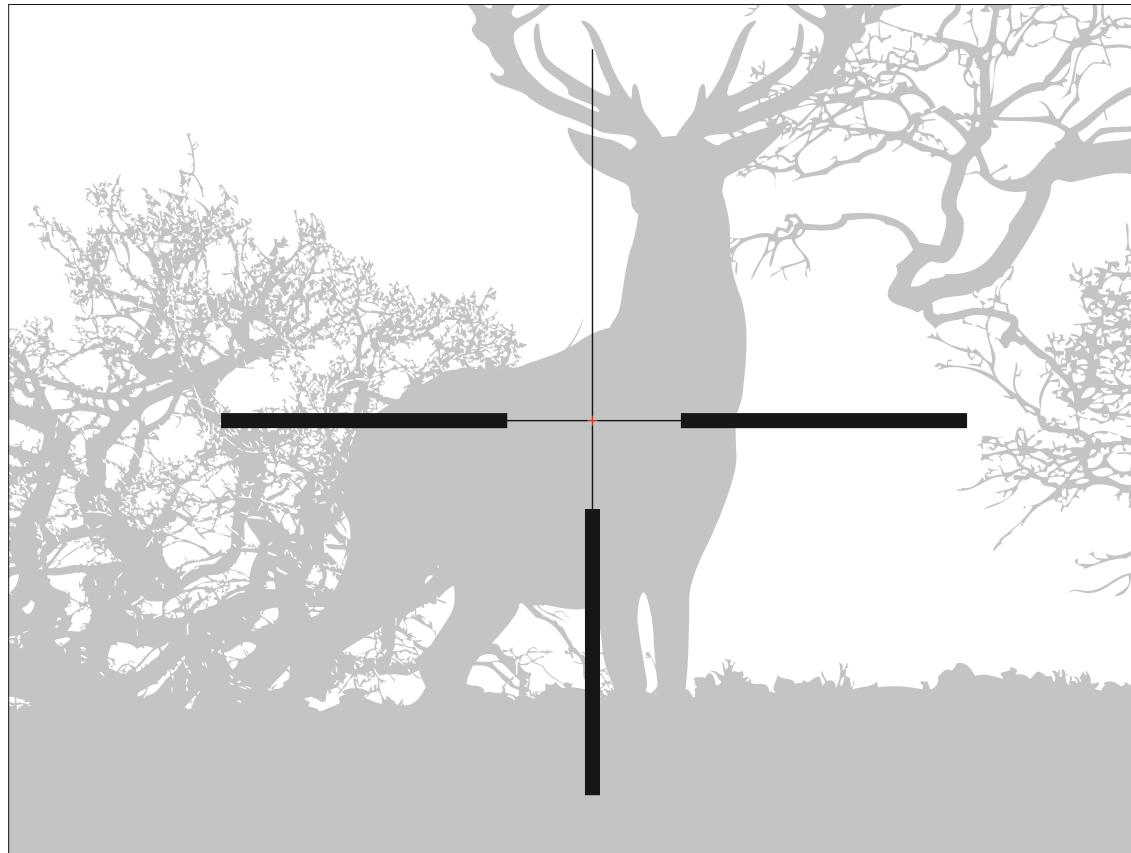

**Reticle parameters**  
(for minimum magnification)

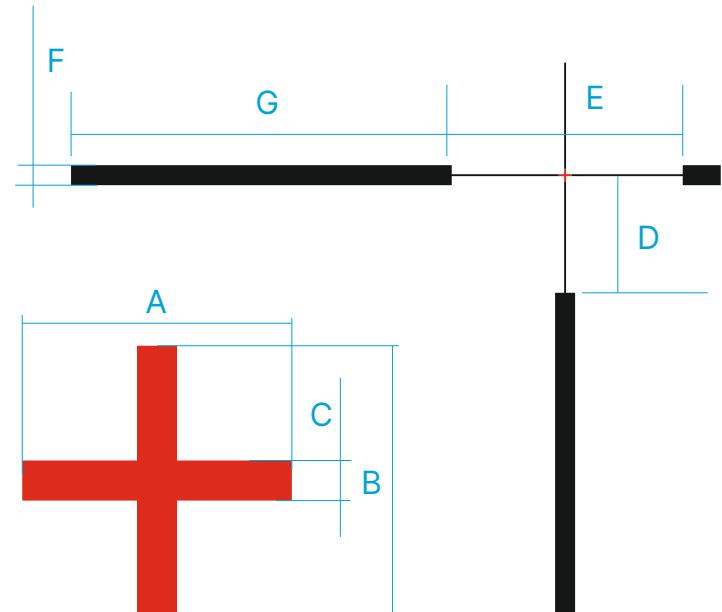

	MOA	cm @ 100 m
Section A	3.1	9
Section B	3.1	9
Section C	0.4	1.2
Section D	17.2	50
Section E	34.4	100
Section F	1.2	3.5
Section G	121	351


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


**TO CONTENT**



# T54

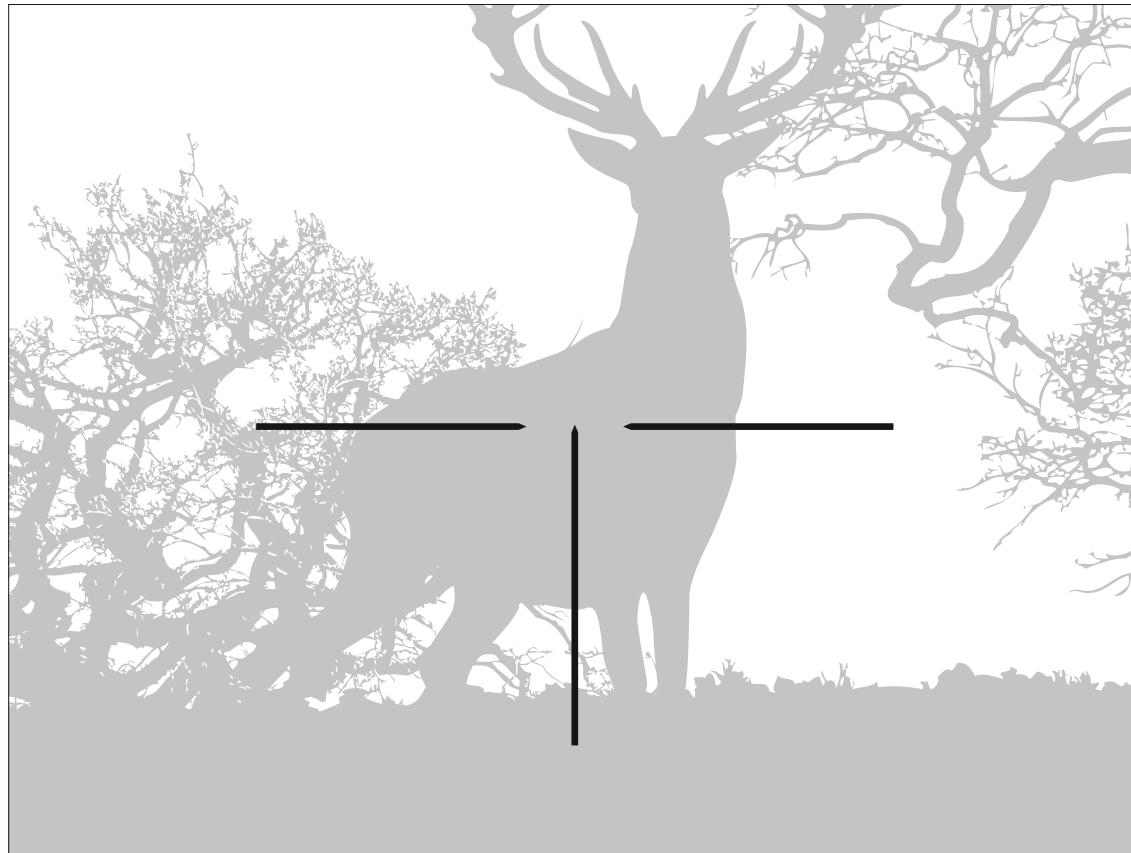

**Reticle parameters**  
(for minimum magnification)

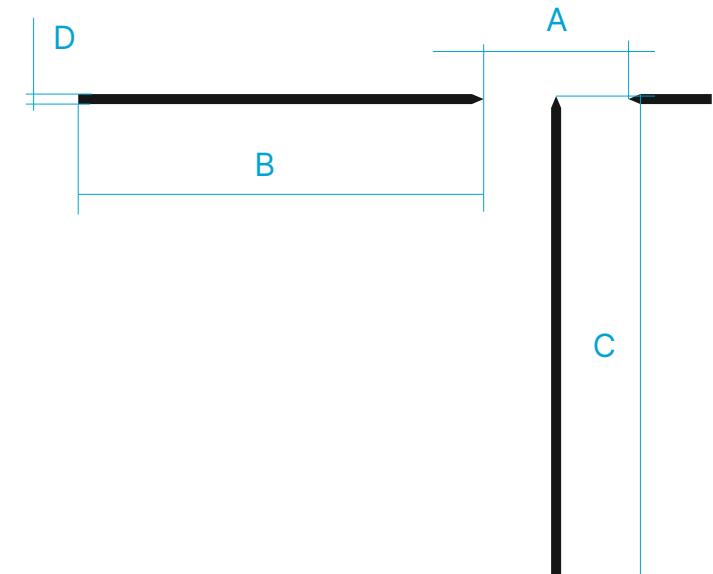

	MOA	cm @ 100 m
Section A	34.4	100
Section B	121	351
Section C	138	402
Section D	3.1	9


Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO


[TO CONTENT](#)



# M58i

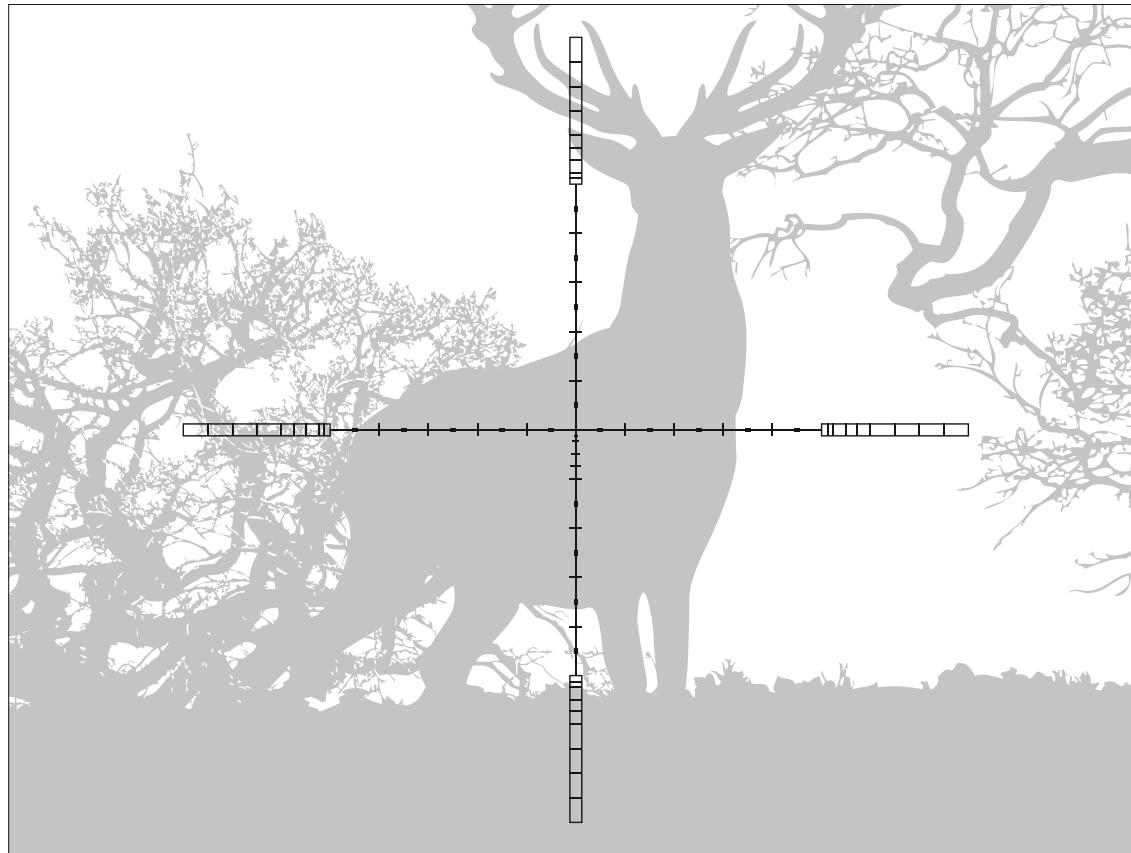

Reticle parameters

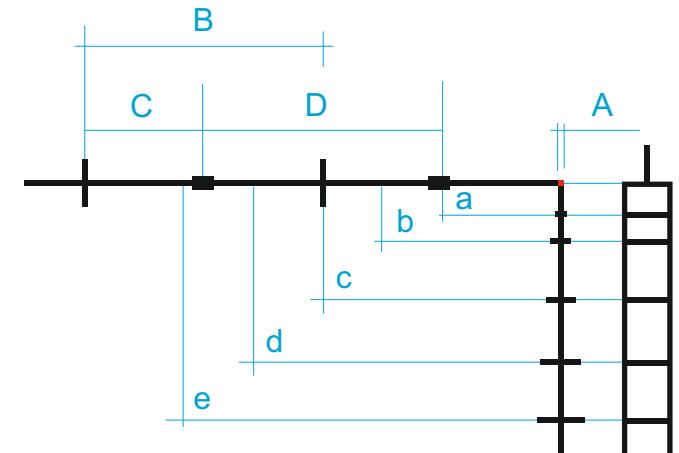

	MOA	cm @ 100 m
Section A	0.4	1.2 on 3x magnification
Section B	3.5	10 (1 mil) on 12x magnification
Section C	3.5	10 (1 mil) on 6x magnification
Section D	3.5	10 (1 mil) on 12x magnification

Section a	1 mil (10 cm @ 100 m) on 3x magnification
Section b	1 mil (10 cm @ 100 m) on 4x magnification
Section c	1 mil (10 cm @ 100 m) on 6x magnification
Section d	1 mil (10 cm @ 100 m) on 9x magnification
Section e	1 mil (10 cm @ 100 m) on 12x magnification

Thermal Imaging Riflescope


## THERMION 2 LRF XQ50 PRO

**TO CONTENT**




# X51 Fi-300

SCALABLE

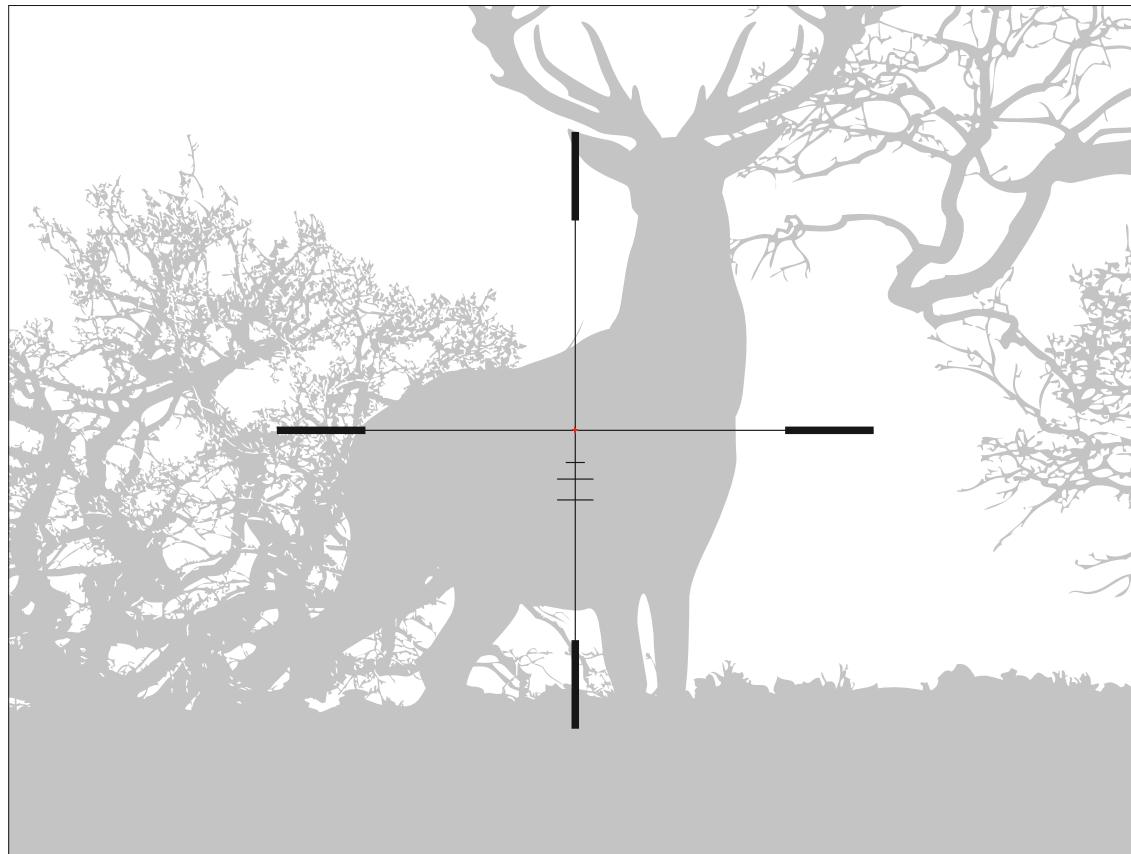

**Reticule parameters**  
(apply to all magnifications)

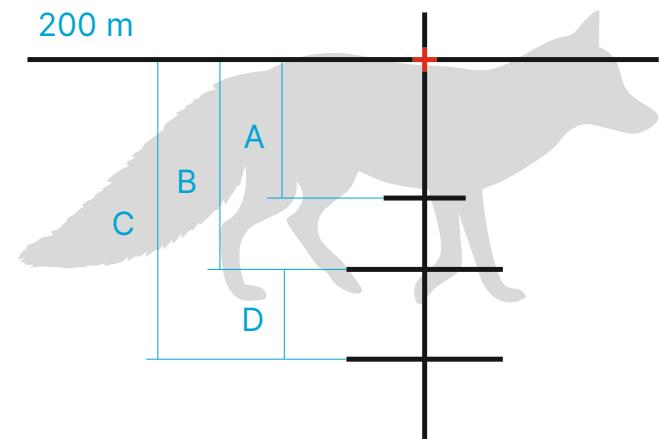

	200 m	300 m
Section A	15 cm (fox body)	23 cm (roe deer body)
Section B	23 cm (roe deer body)	35 cm (wild boar body)
Section C	35 cm (wild boar body)	50 cm (deer body)
Section D	—	15 cm (fox body)

Thermal Imaging Riflescope


## THERMION 2 LRF XQ50 PRO

TO CONTENT




# M56Fi

SCALABLE

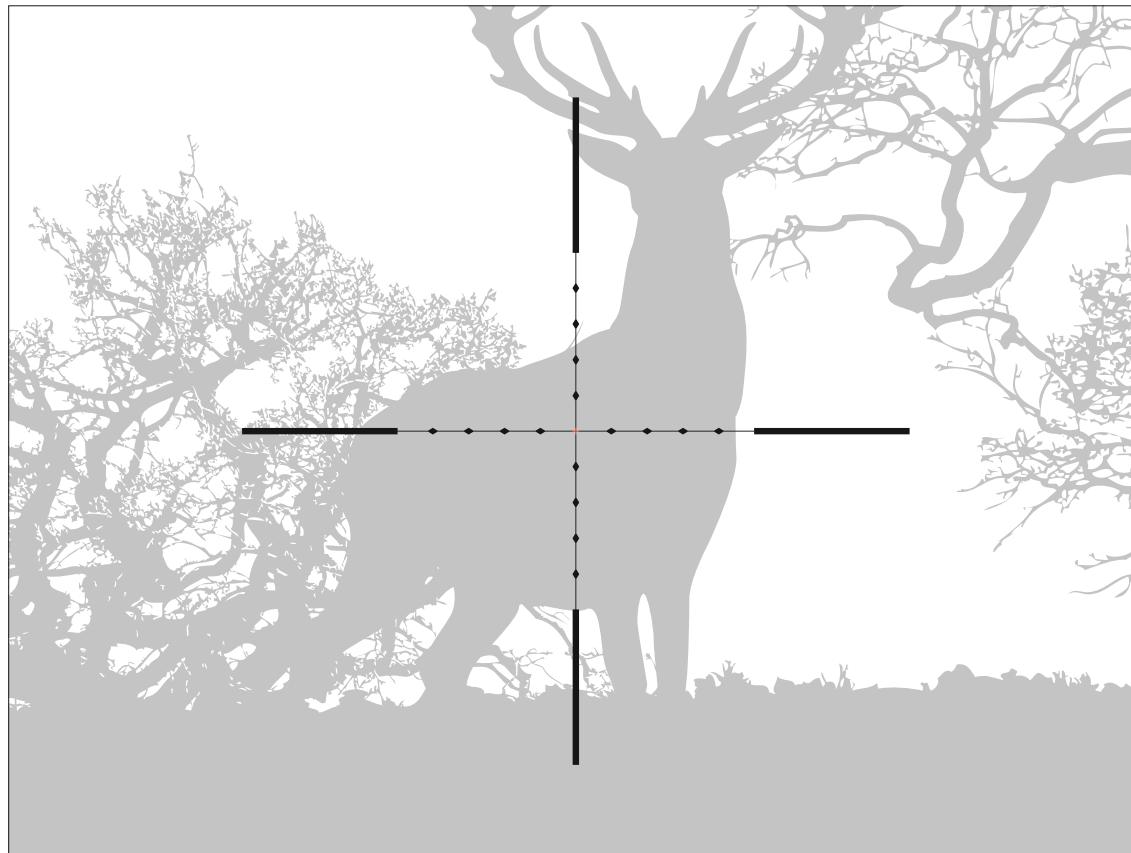

**Reticule parameters**  
(apply to all magnifications)

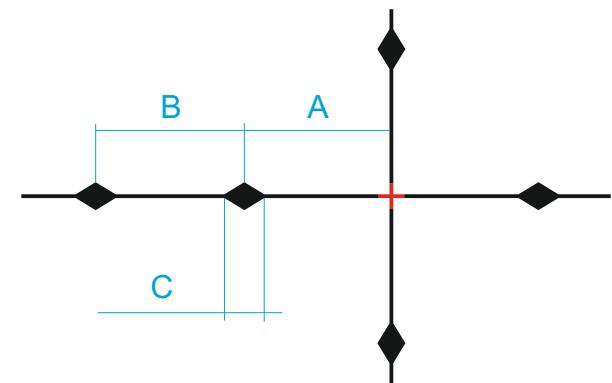

	MOA	CM @ 100 M
Section A	3.5	10 (1 MIL)
Section B	3.5	10 (1 MIL)
Section C	0.86	2.5 (0.25 MIL)

Thermal Imaging Riflescope


## THERMION 2 LRF XQ50 PRO

[TO CONTENT](#)




# M57Fi

SCALABLE

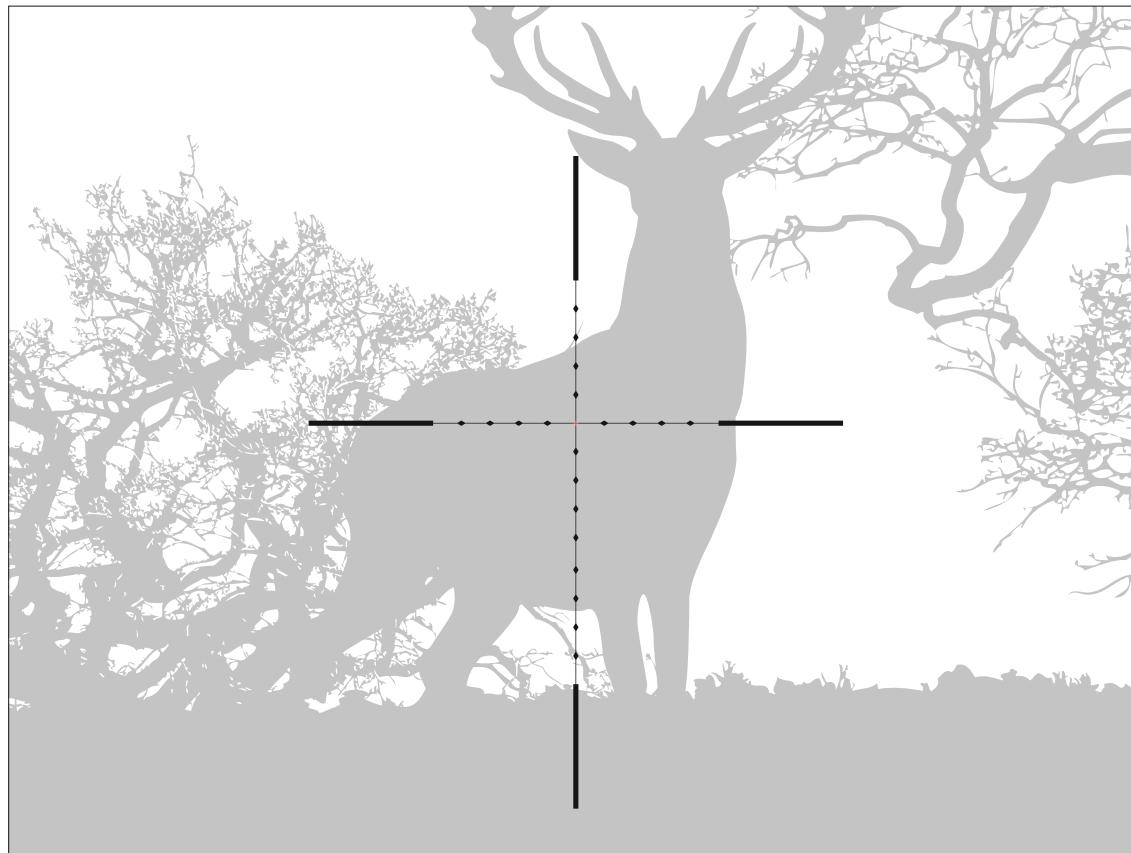

**Reticule parameters**  
(apply to all magnifications)

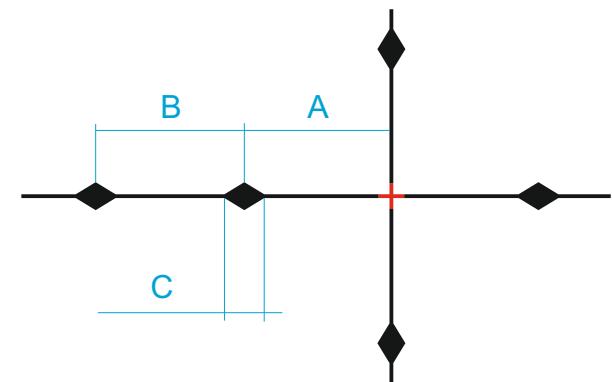

	MOA	CM @ 100 M
Section A	3.5	10 (1 MIL)
Section B	3.5	10 (1 MIL)
Section C	0.86	2.5 (0.25 MIL)

Thermal Imaging Riflescope

## THERMION 2 LRF XQ50 PRO

[↑ TO CONTENT](#)



[www.pulsar-vision.com](http://www.pulsar-vision.com)